

RTX1 Transmitter for the SDX-15 Plant Alarm System

About this manual.



When you see this symbol, the associated text in bold type refers to something which may cause danger or damage.


Transmitters introduce signals from plant etc. onto the multiplexed signal wiring. The RTX1 is designed to be mounted within the same enclosure as the alarm contacts when used for medical applications, as cable monitoring is not used.

The RTX1 is a self contained unit, used where indication of the alarm condition is not required locally, e.g. when a manifold or plant has an integral plant to alarm interface, and is available as a one gas (4 condition) unit. The service is selected, as in the alarm panel, with a rotary switch. Each service on the system is allocated a channel when the system is initially set up, this being entered on the log sheet. The alarm contacts on the plant or manifold are connected to the transmitter as follows:-C Common 1 First condition 2 Second condition 3 Third condition 4 Forth condition For example, if Oxygen is allocated channel 1, this plant could be connected to the alarm input terminals on the transmitter, which would then be set to channel 1. Any condition not transmitted from this transmitter must be linked out to set the condition to normal if the condition is not to be used, or left open circuit if the condition is to be transmitted from another transmitter. It is important to ensure that any condition is only transmitted from one location although other conditions on the service may be transmitted from other transmitters.

The red System Fault LED will flash if the RTX1 does not see the signals from the central alarm on the system, either because of a cable fault or because no central alarm is installed. In this case, all alarm conditions will default to alarm.

WARNING. This equipment is not suitable for connection to an IT power system. A readily accessible means of disconnecting the supply must be provided. The maximum prospective fault current must not exceed 1500 amps A 240 volt, 50/60 Hertz supply is required, which is connected to the mains supply terminals . The 2 core inter-panel wiring is connected to signal terminals 1 & 2. The cable screen must be connected to earth.



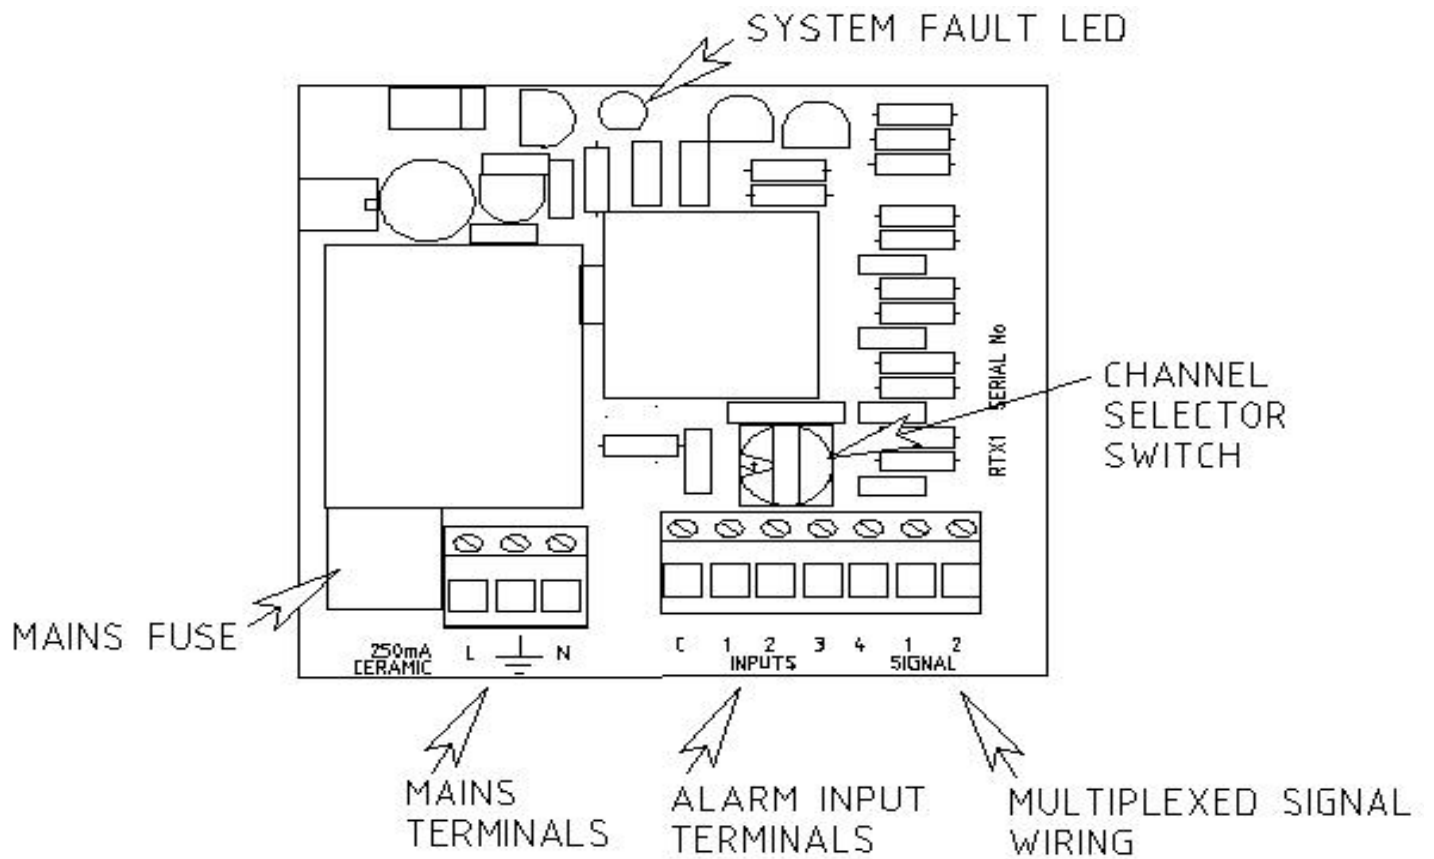

Declaration Of Conformity

2004/108/EG The EMC Directive
2006/95/EG The Low Voltage Directive

Manufacturer

Shire Controls Ltd
Studio 3, Channoeks Farm
Gilston, Harlow
Essex CM202RL
United Kingdom

Product Type

RTX1 Remote Transmitter

Year of manufacture 2018

Standards used

BSEN61000-6-3:2007+A1:2011
BSEN61000-6-1:2007
BSEN61000-3-2:2014
BSEN60950-1:2006

Authorised representative

I.R.Couchman Technical Director
Signature